



1/12

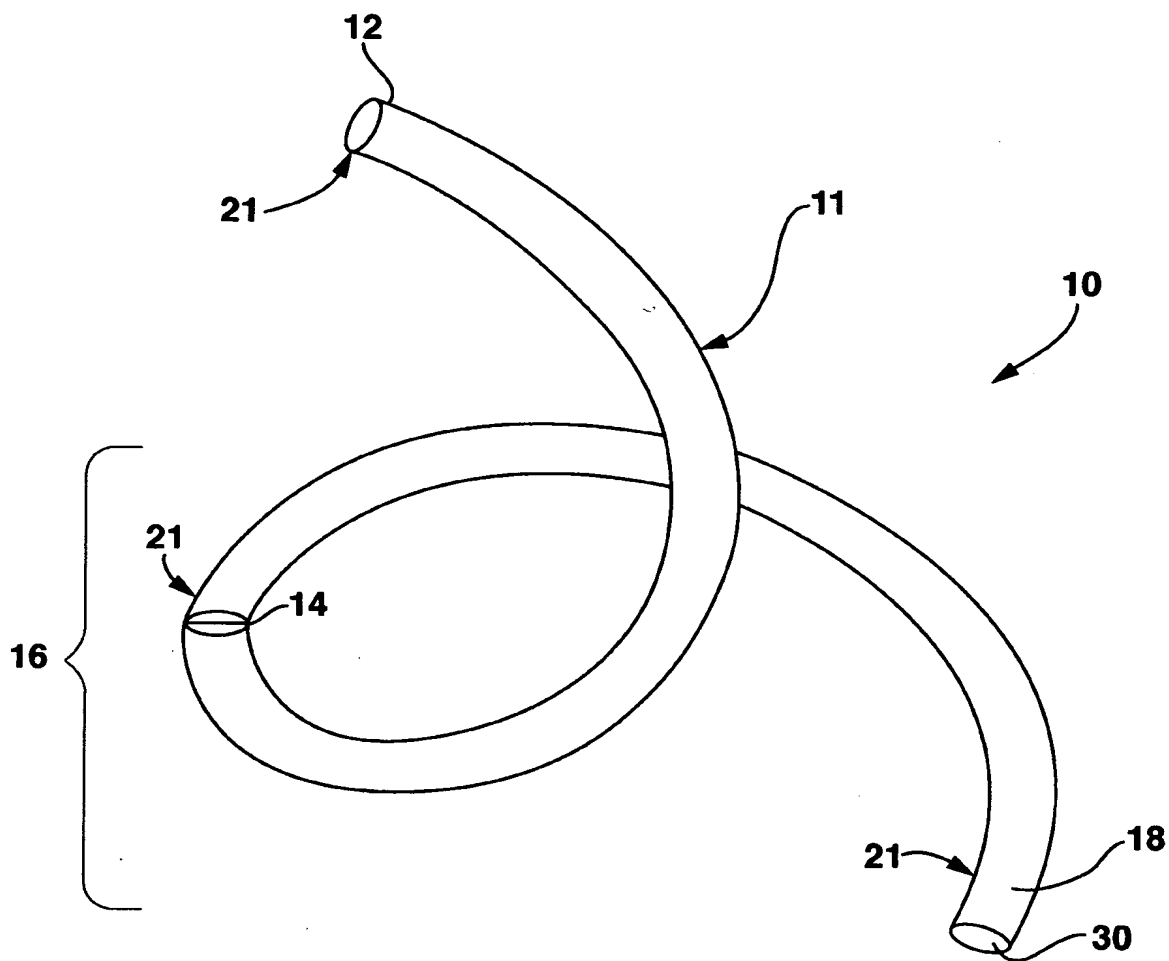


FIG. 1

2/12

FIG. 3


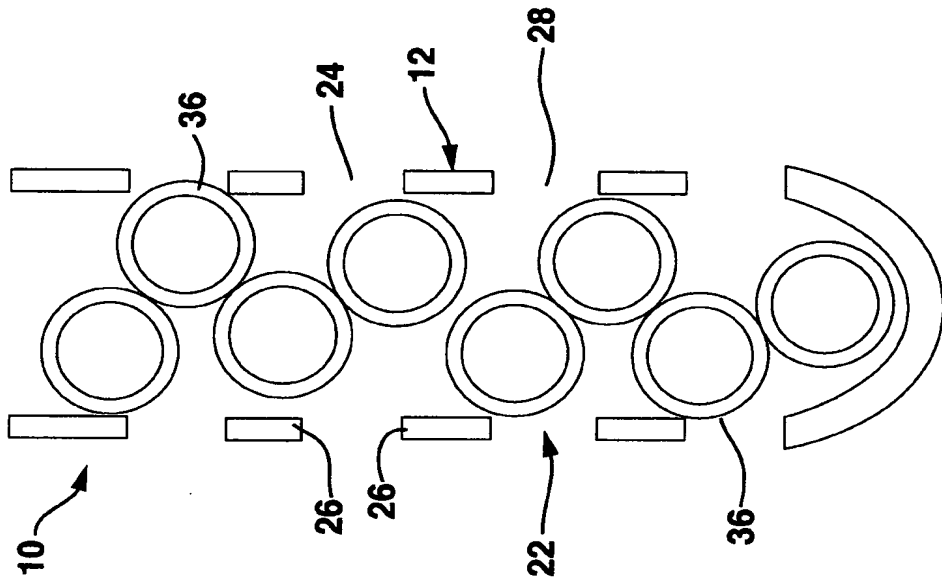


FIG. 2

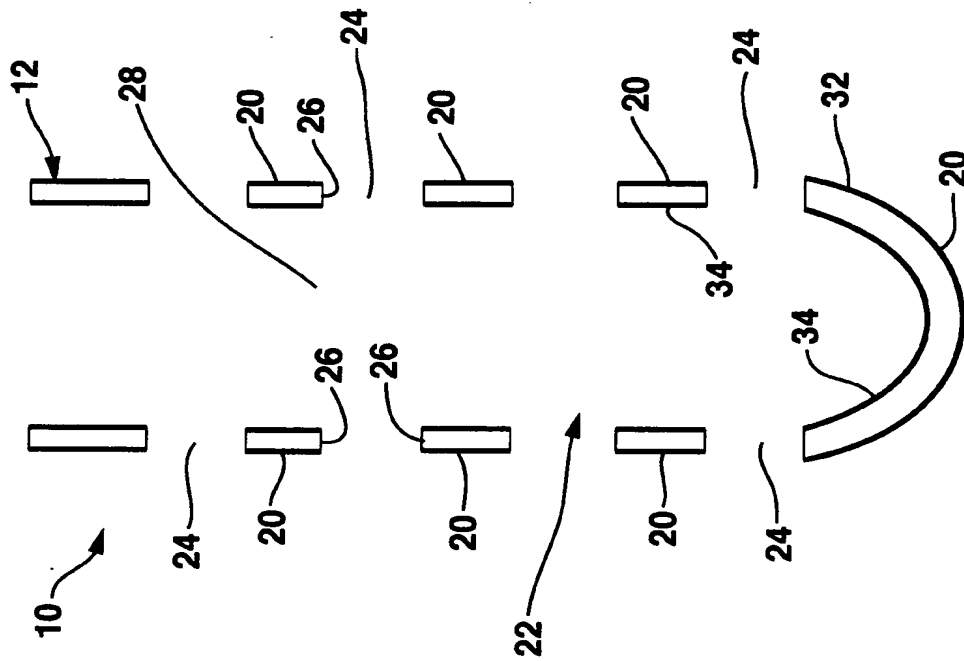

3/12

FIG. 5


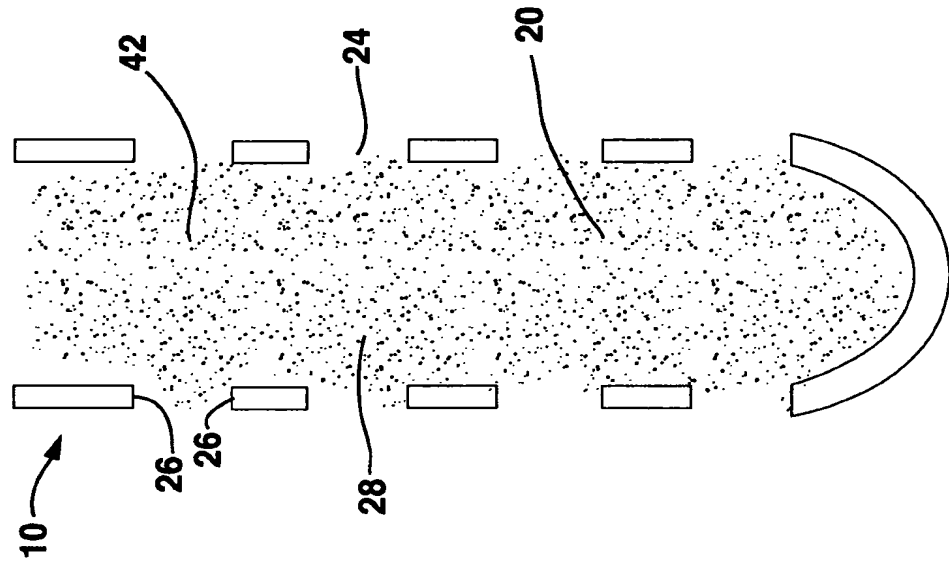


FIG. 4

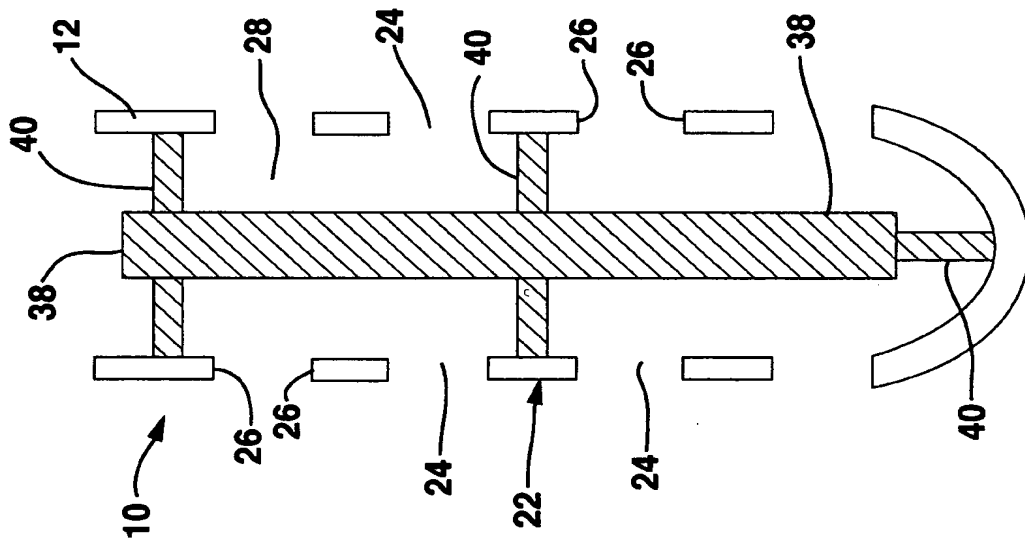

4/12

FIG. 7







FIG. 6

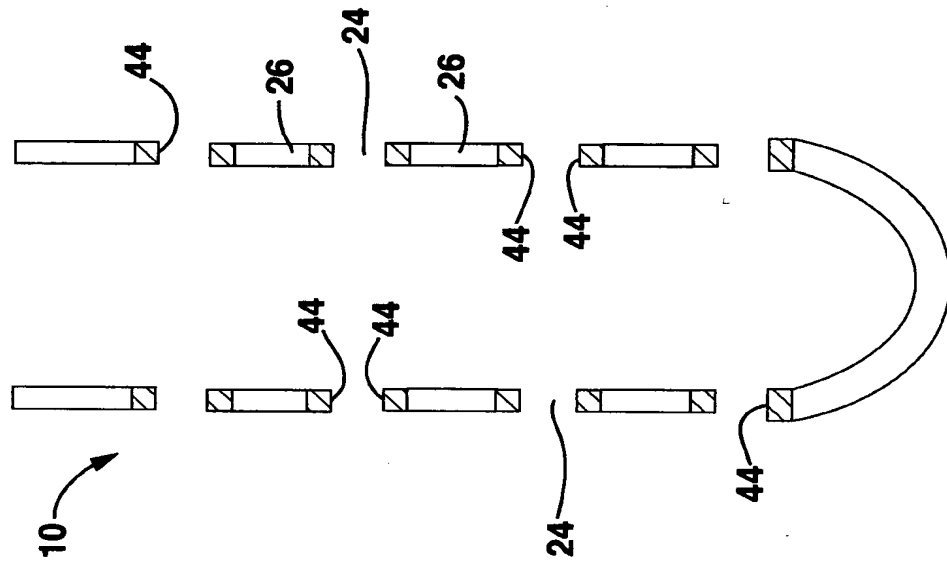


5/12

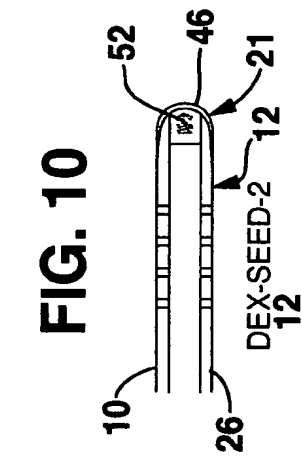


**FIG. 10**

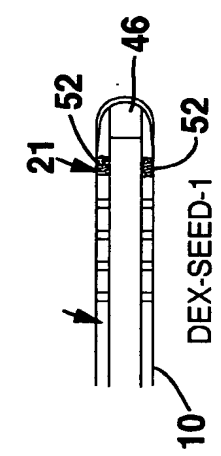


**FIG. 11**

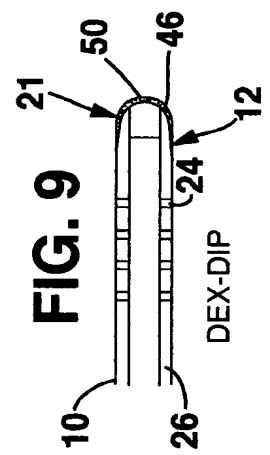


**FIG. 9**

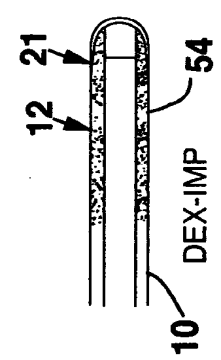


**FIG. 12**

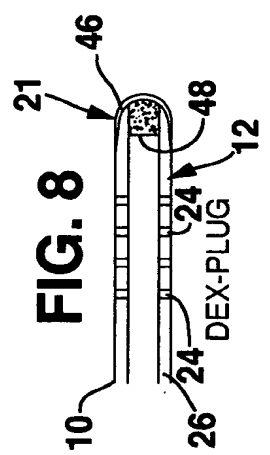

**FIG. 8**

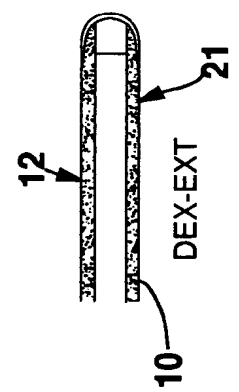

**FIG. 13**

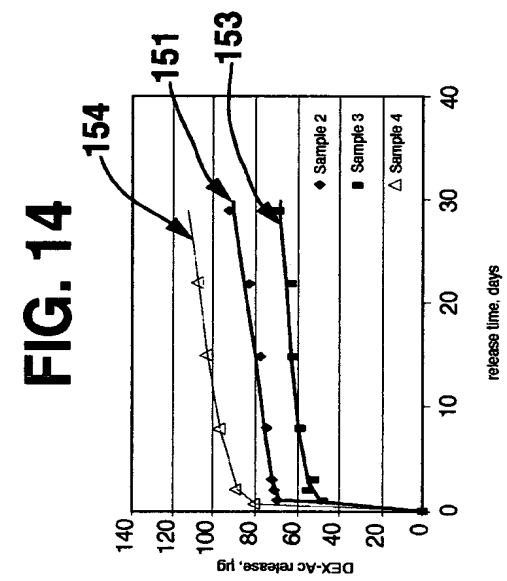

**FIG. 14**

6/12

FIG. 15



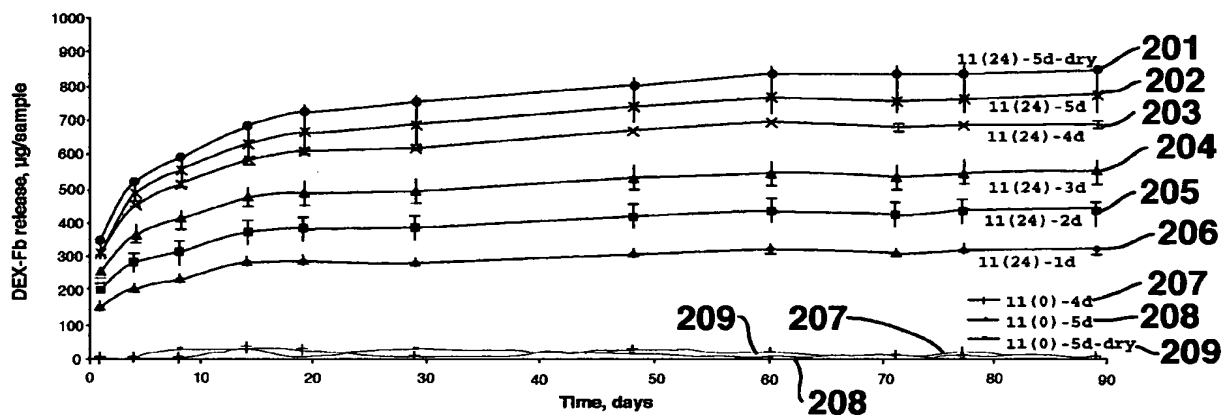


FIG. 16

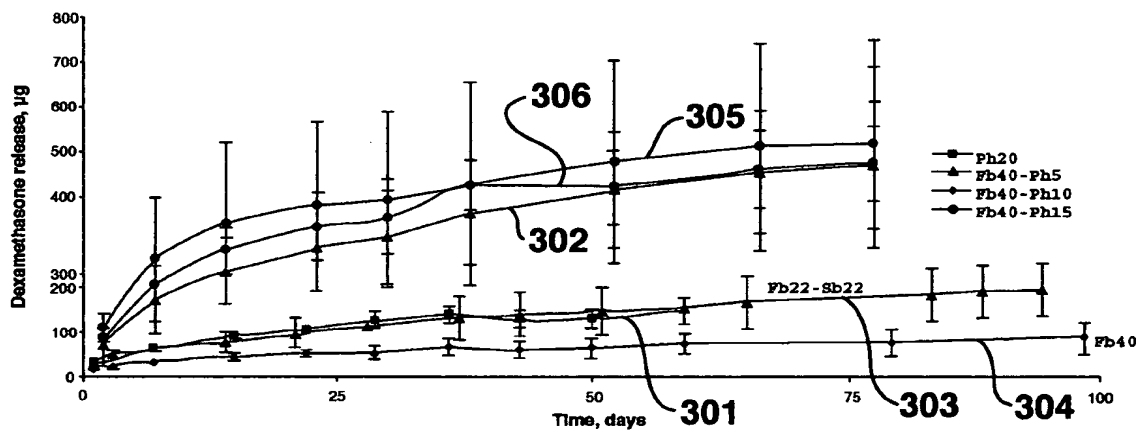


7/12

**FIG. 17**

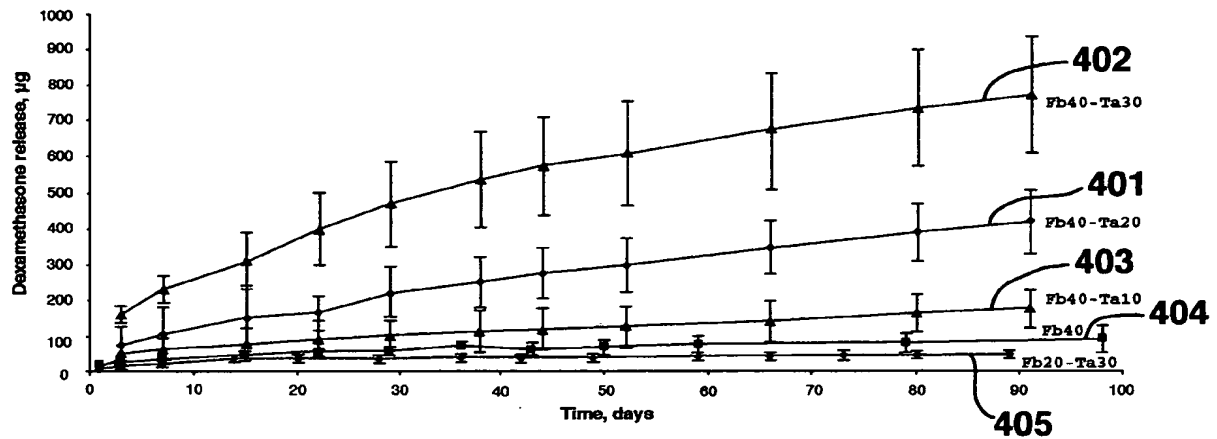

**FIG. 18**

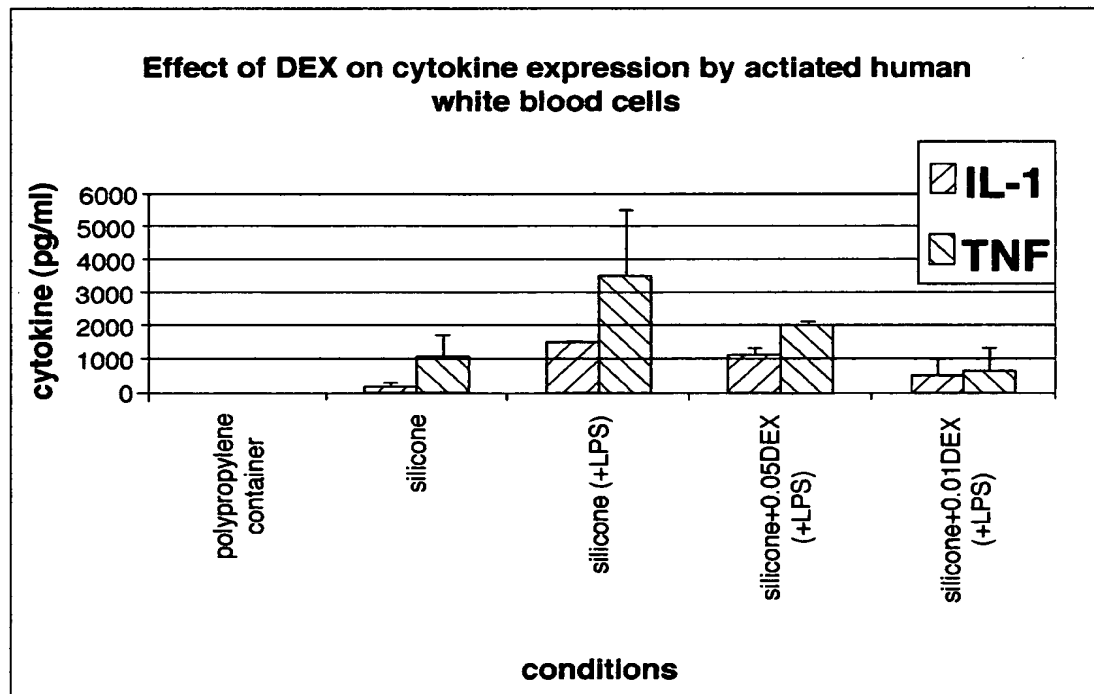

8/12

FIG. 20

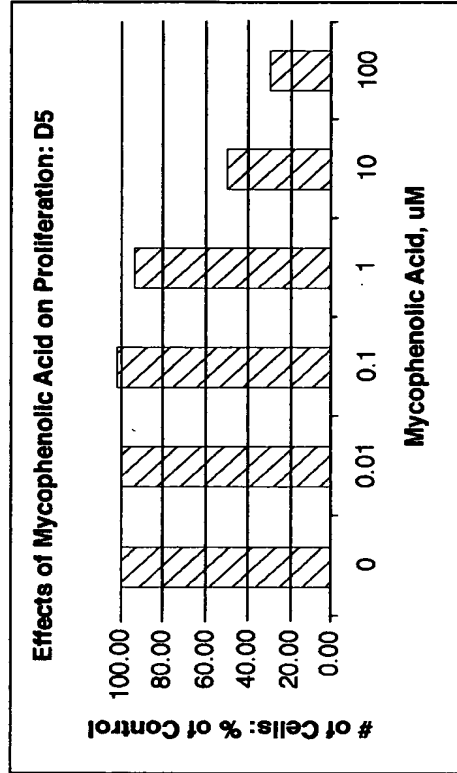


FIG. 19

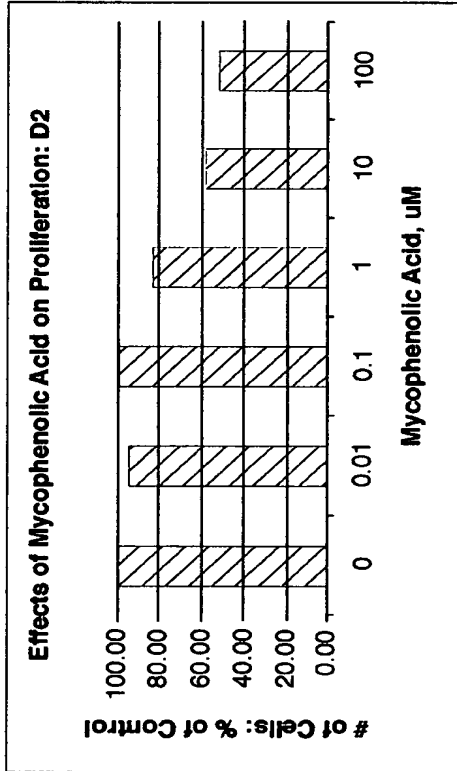


FIG. 22


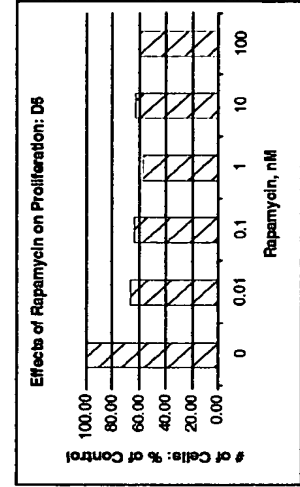


FIG. 21



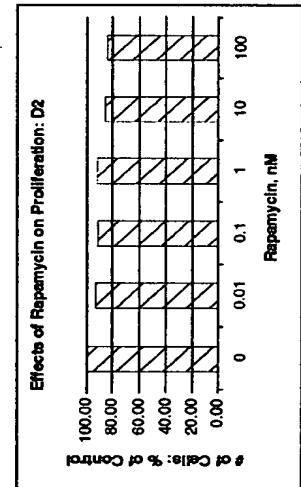

9/12

FIG. 28

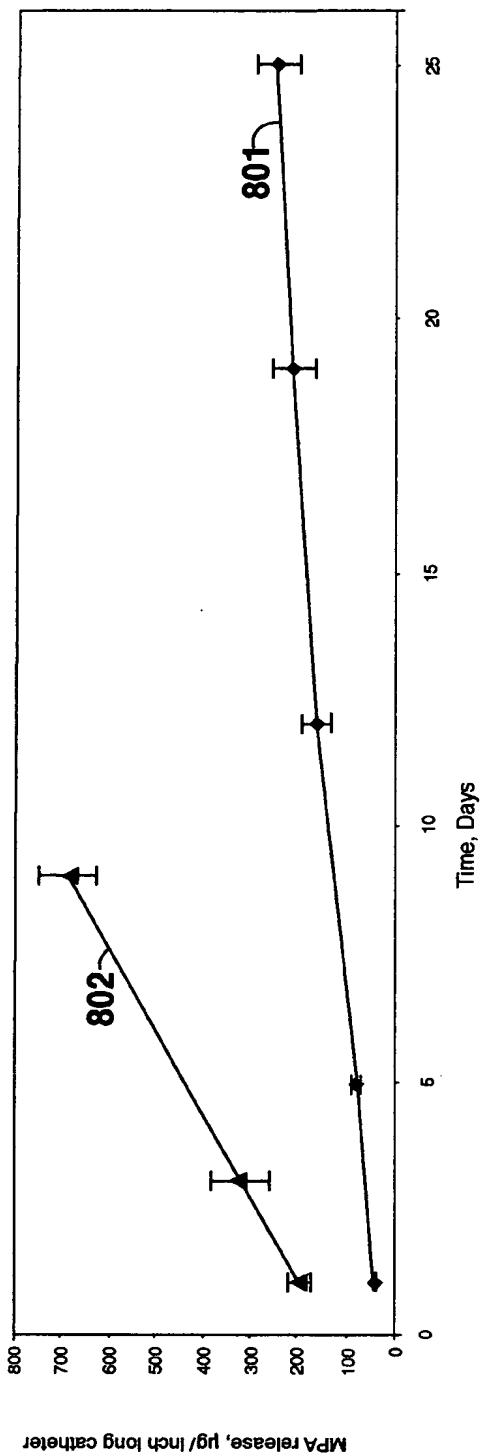


FIG. 24


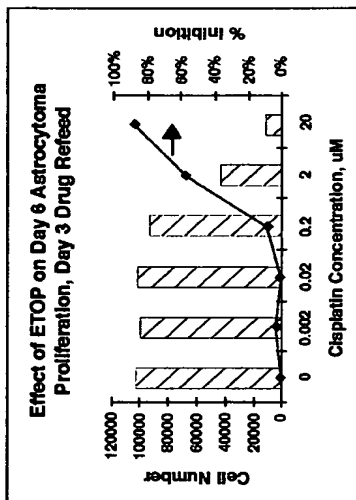


FIG. 23

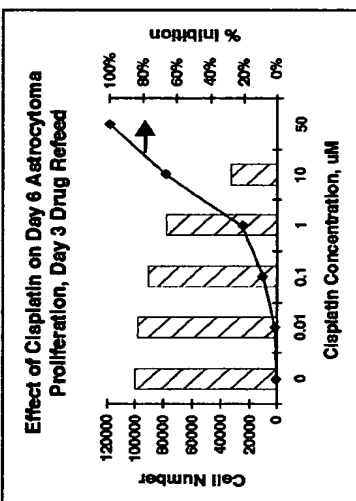

10/12

FIG. 25



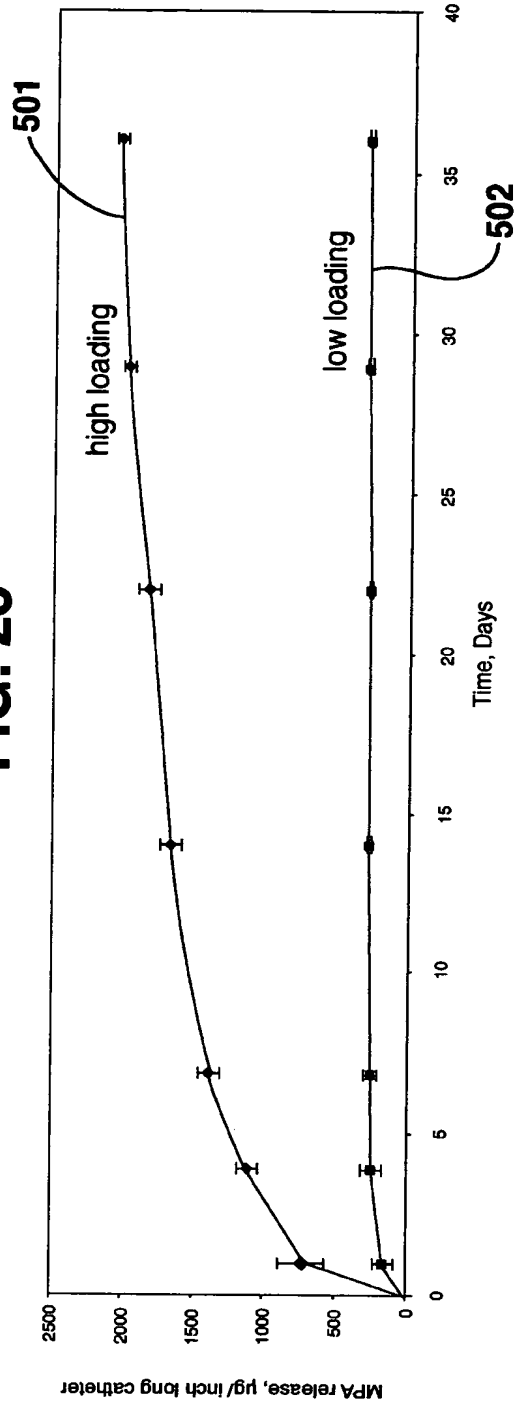


FIG. 26

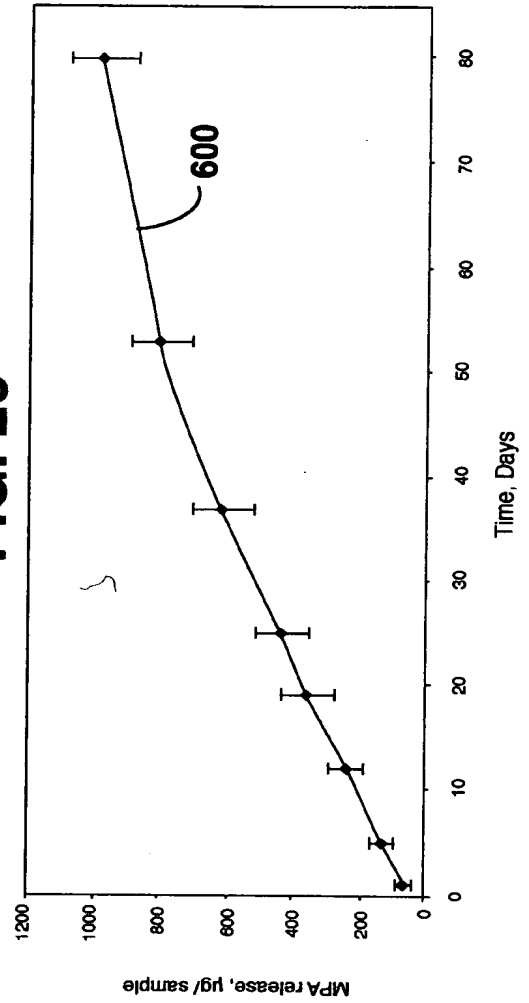


11/12

FIG. 27

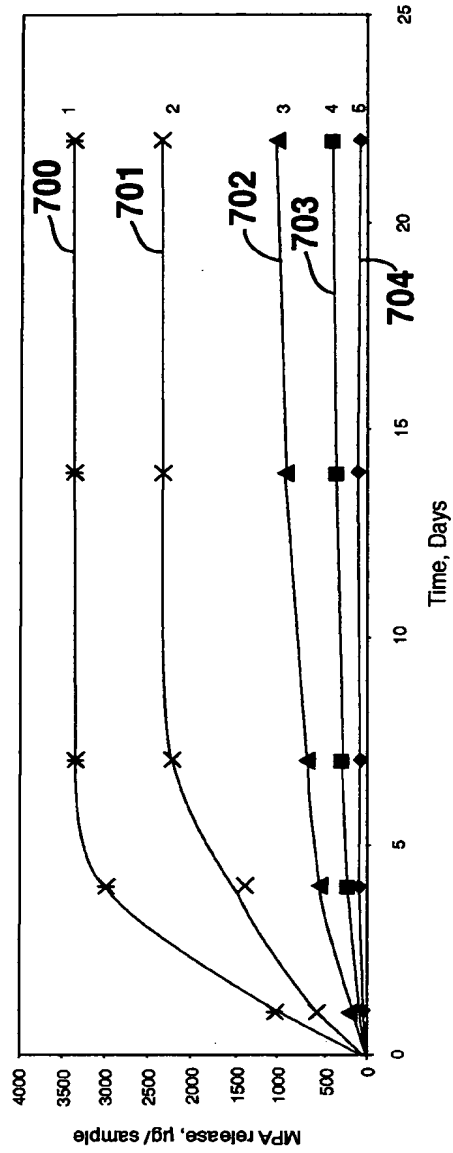

12/12

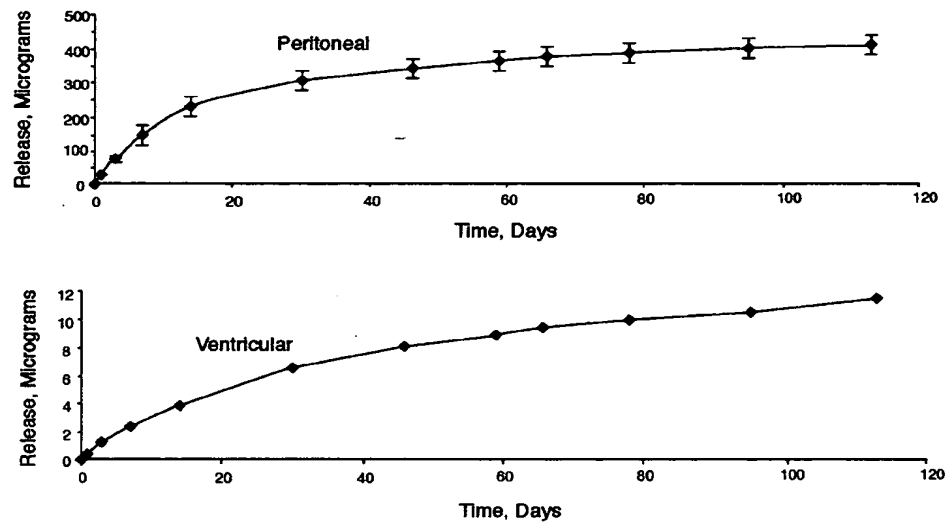

In-vitro release of RAPA from silicone catheters of different sizes.

**FIG. 29**